



Under Test: TC4013-4
S/N: 2018075
Reference: TC4033
Date: 2018-10-05
Session, Run: 30692, 1
Max RR: -210.4 dB re 1 μ Pa/V at 1m
SL Right: -0.0°, -0.0dB dB re 1 μ Pa/V at 1m
Comment: Horizontal.

HYDROPHONE DIRECTIVITY

Amplitude: 20.0 Vrms
Pulse Width: 150.0 μ s
Angle: -180.0° to 180.0°
Frequency: 100.00 kHz

PR10.2 (2 de 12) Description des travaux 2020




Temperature: 21.21°C
Depth: 1.2 m
Distance: 0.50 m
Tested by: PRA

15 OKT. 2018

FAN OK

For all mats!
2018-10-11 PRA

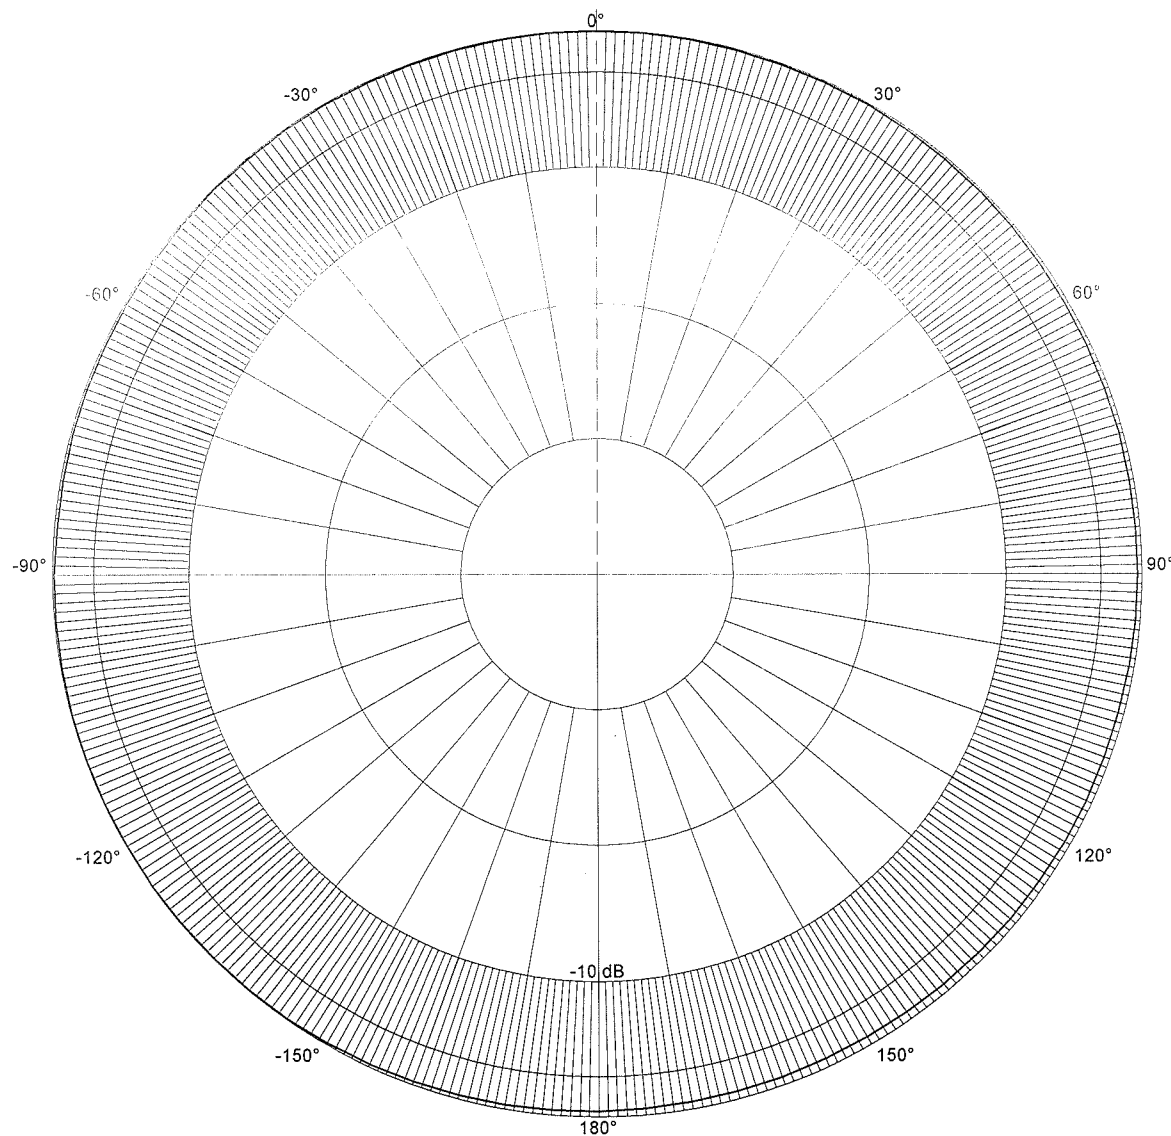




Under Test: TC4013-4
S/N: 2018075
Reference: TC4033
Date: 2018-10-11
Session, Run: 30730, 2
Max RR: -210.3 dB re 1 μ Pa/V at 1m
W: 342.8°
Comment: Vertical.

HYDROPHONE DIRECTIVITY

Amplitude: 10.0 Vrms
Pulse Width: 150.0 μ s
Angle: -180.0° to 180.0°
Frequency: 100.00 kHz

Temperature: 21.32°C
Depth: 1.2 m
Distance: 0.50 m
Tested by: PRA

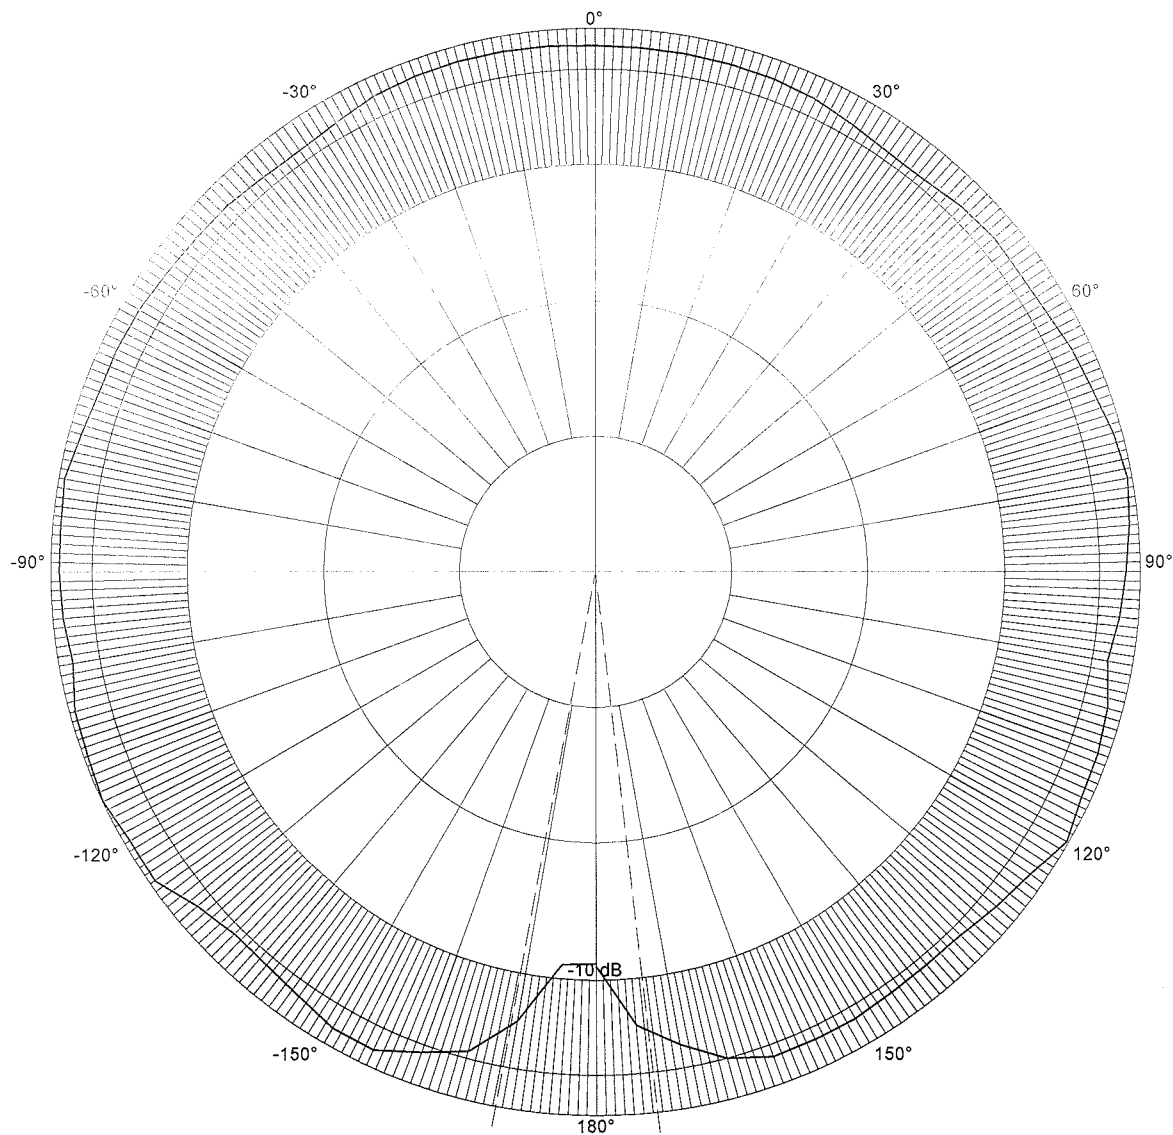




HYDROPHONE SENSITIVITY

Under Test: TC4013-4
S/N: 2018075
Reference:
Date: 2018-10-05
Session, Run: 30692, 2
Comment: PHO @ 250 Hz: -211.8 dB.

Amplitude: 25.0 Vrms
Pulse Width: 1400.0 μ s
Rep Rate: 66.7 ms
Averages: 8

Temperature: °C
Depth: 0.0 m
Distance: 0.00 m
Tested by: PRA

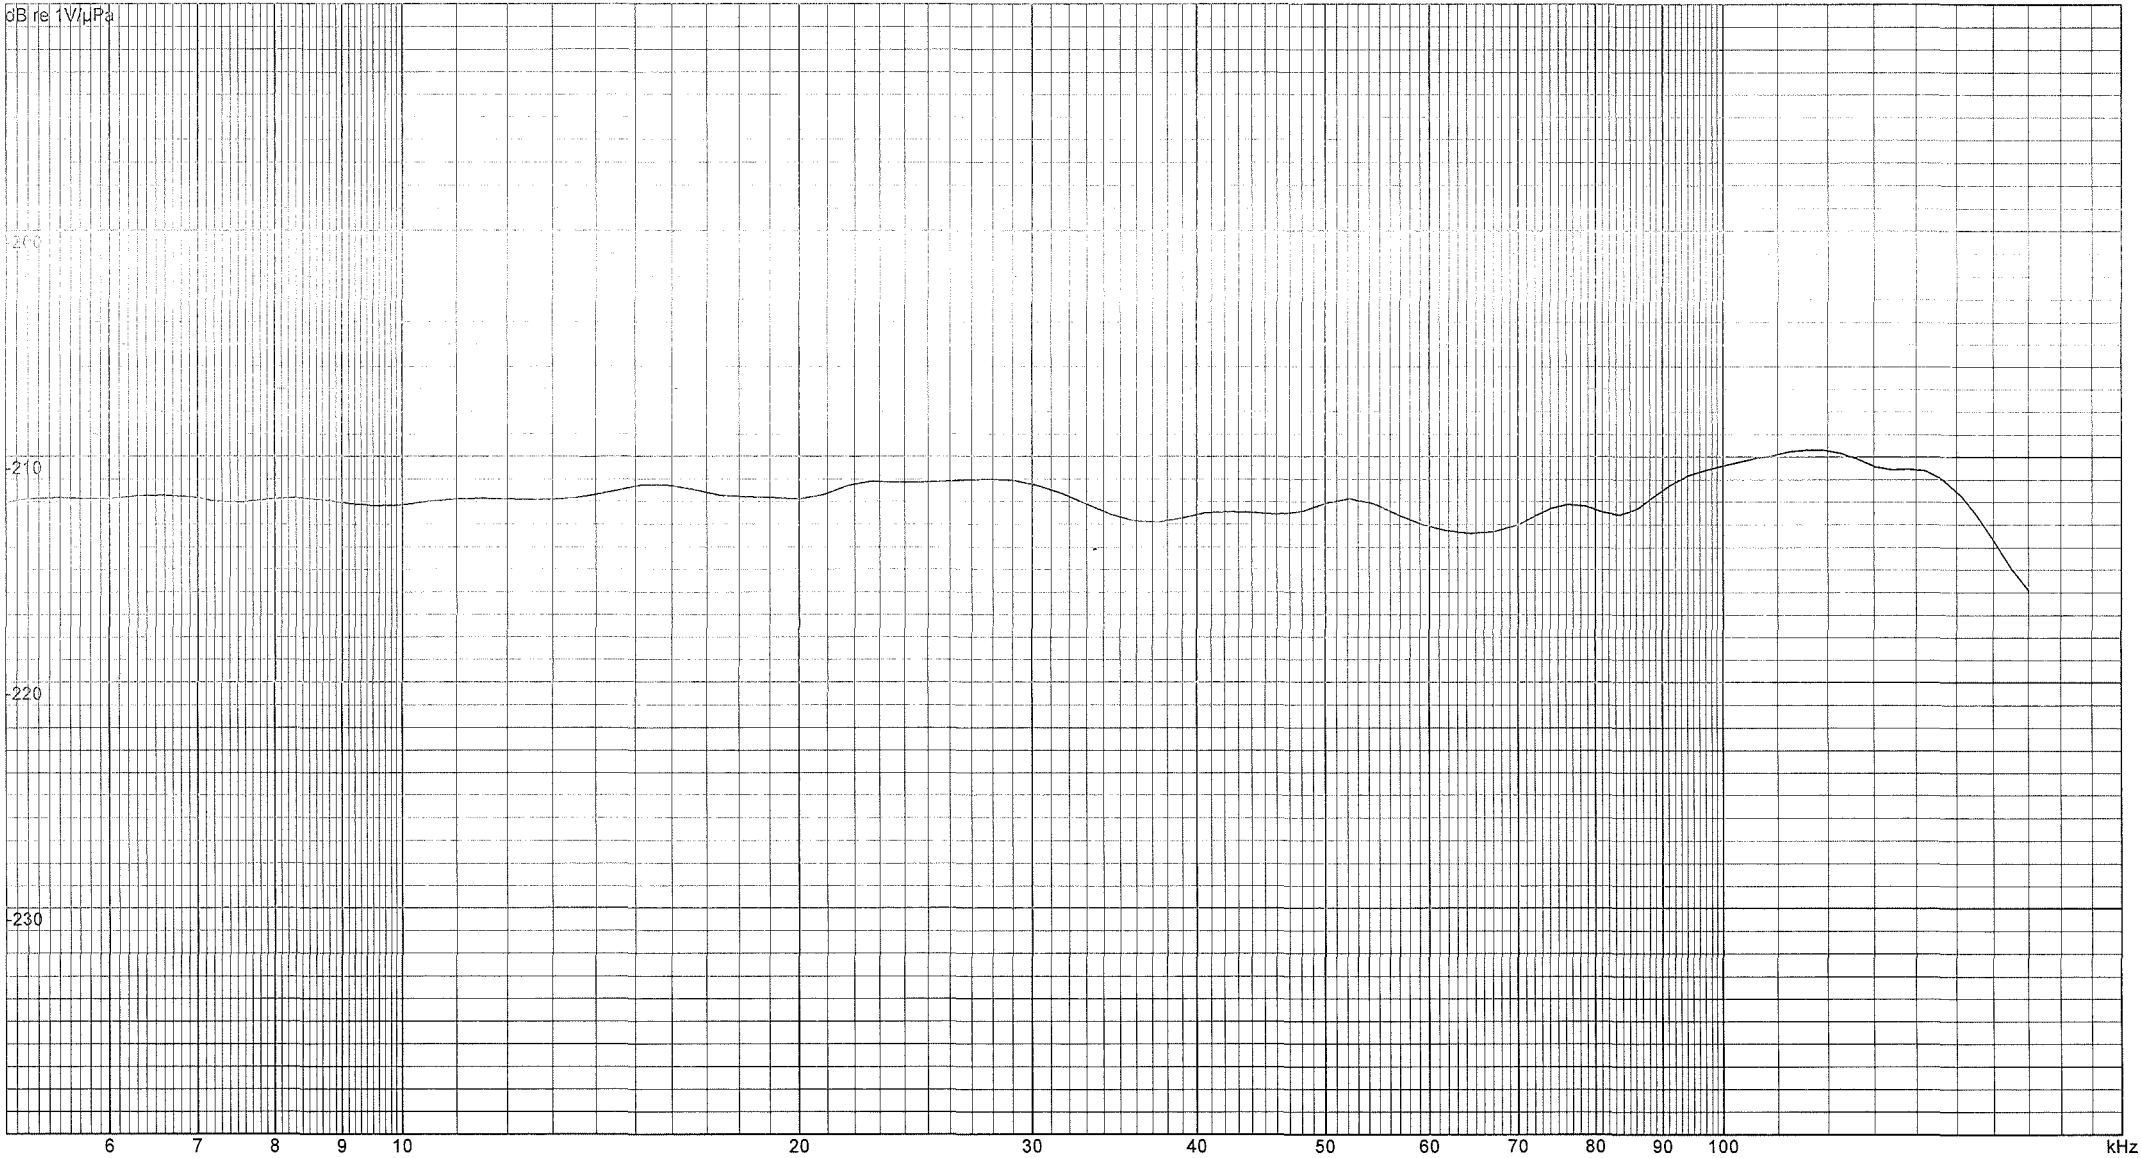




Under Test: TC4013-4
S/N: 2018075
Reference:
Date: 2018-10-05
Session, Run: 30692, 5
100.00 kHz: 132.29 dB re 1 μ Pa/V at 1m
Comment:

PROJECTOR SENSITIVITY

Amplitude: 20.0 Vrms
Pulse Width: 1400.0 μ s
Rep Rate: 100.0 ms
Averages: 8

Temperature: °C
Depth: 0.0 m
Distance: 0.00 m
Tested by: PRA

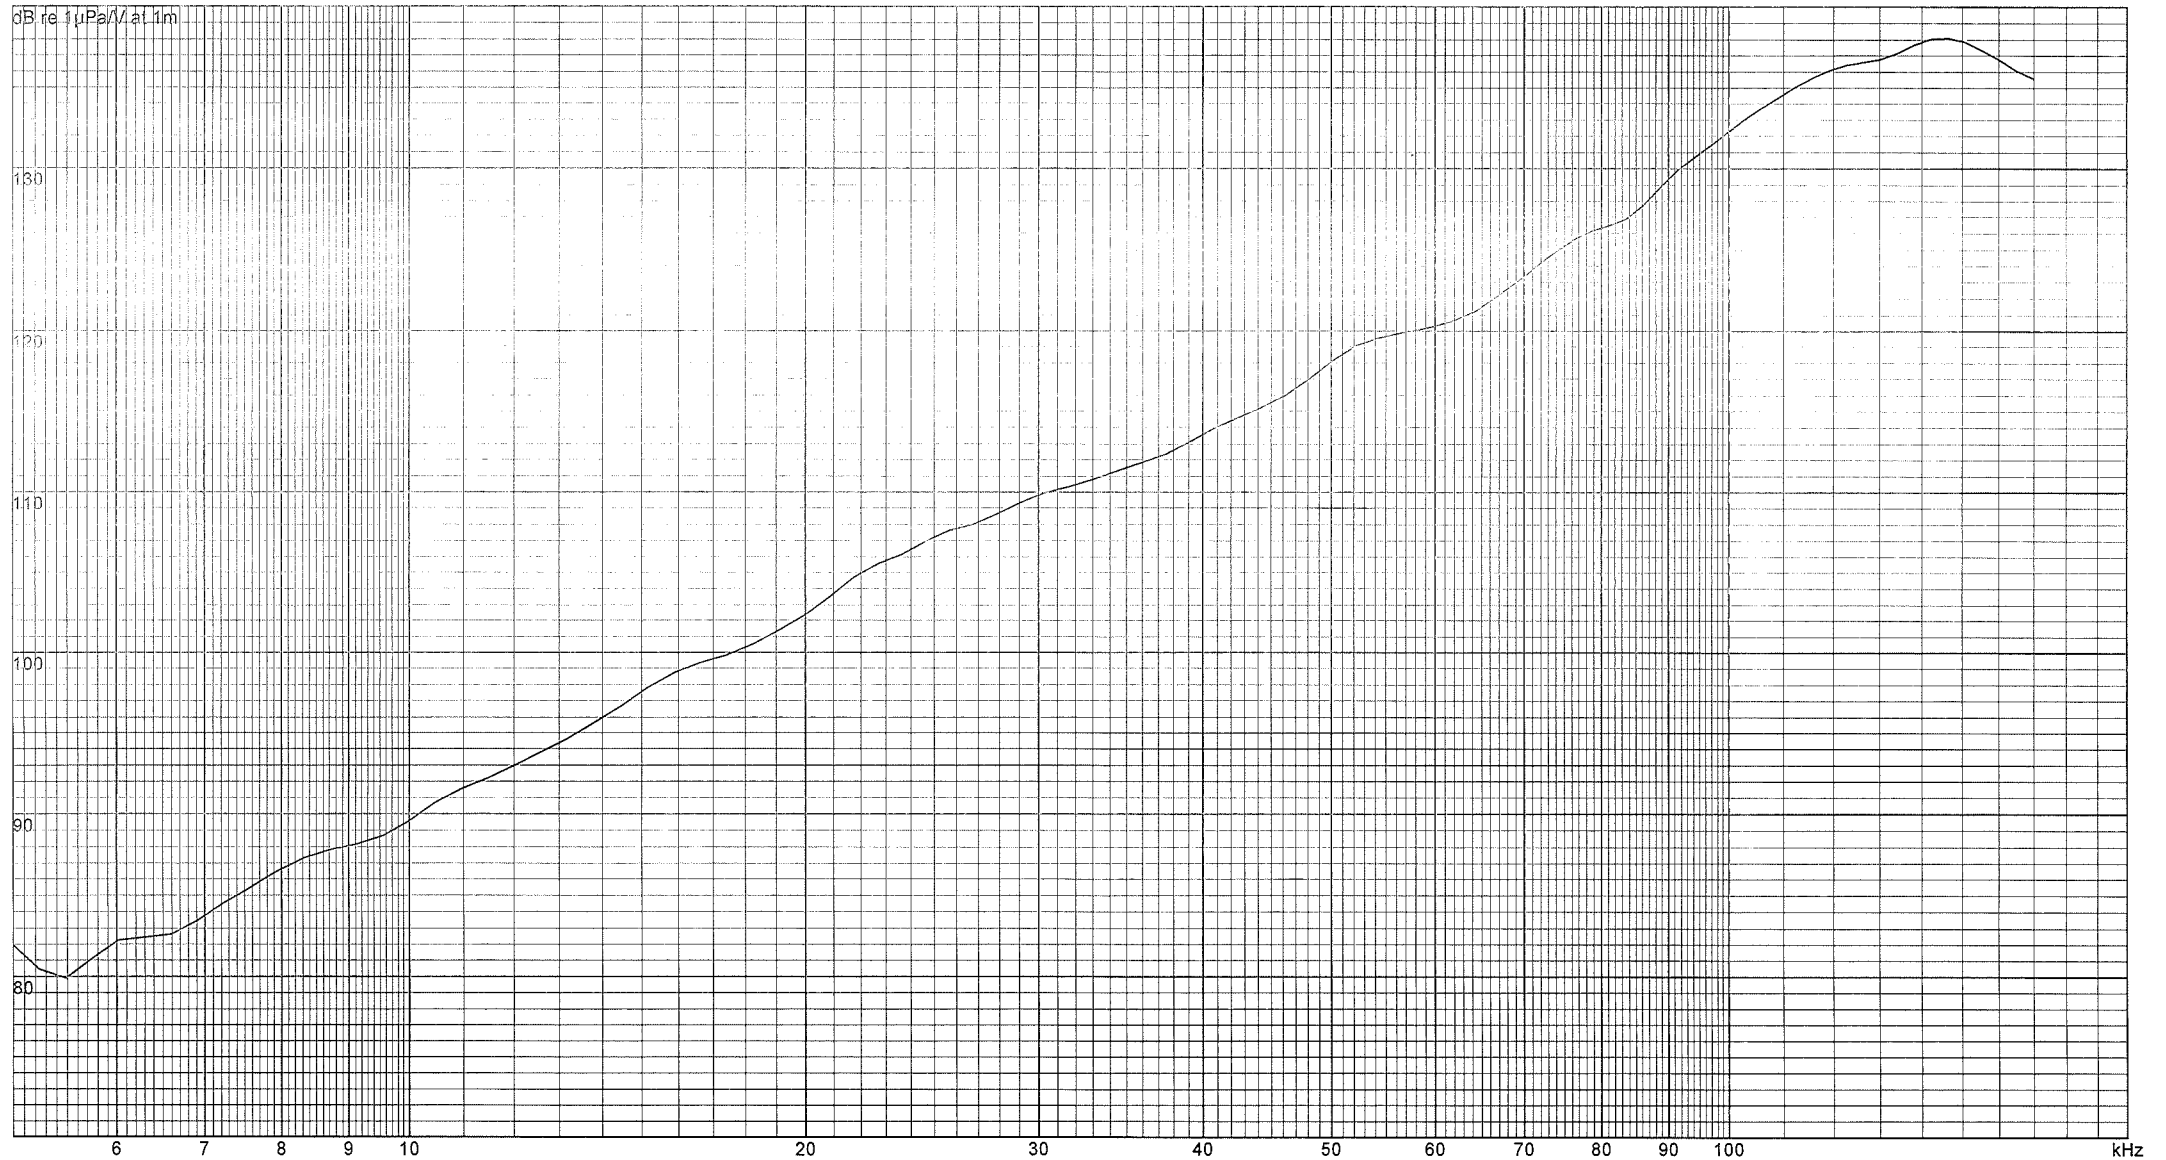



Under Test: TC4013-4
S/N: 2018075
Date: 2018-10-05
Session, Run: 30692, 6
Comment:

IMPEDANCE SUMARY

Amplitude: 10.0 Vrms
Pulse Width: 3000.0 μ s
Rep Rate: 33.3 ms
Averages: 4

Temperature: 21.21°C
Depth: 1.2 m
Cal Resistor: 0.0 ohms
Tested by: PRA

—— 2018075\Impedance\1\Impedance\Try 1
----- 2018075\Impedance\1\Resistance\Try 1
..... 2018075\Impedance\1\Reactance\Try 1

