



HYDROPHONE DIRECTIVITY

PR10.2 (4 de 12) Description des travaux 2020

Under Test: TC4013-4
S/N: 0515084
Reference: TC4033
Date: 2015-04-01
Session, Run: 22116, 1
Max RR: -210.8 dB re 1 μ Pa/V at 1m
SL Right: -85.0°, 0.0dB dB re 1 μ Pa/V at 1m
Comment: Horizontal.


Amplitude: 20.0 Vrms
Pulse Width: 150.0 μ s
Angle: -180.0° to 180.0°
Frequency: 100.00 kHz

Temperature: 21.72°C
Depth: 1.2 m
Distance: 0.50 m
Tested by: PRA

07 APR 2015

For all parts!

2015-04-01 PRA

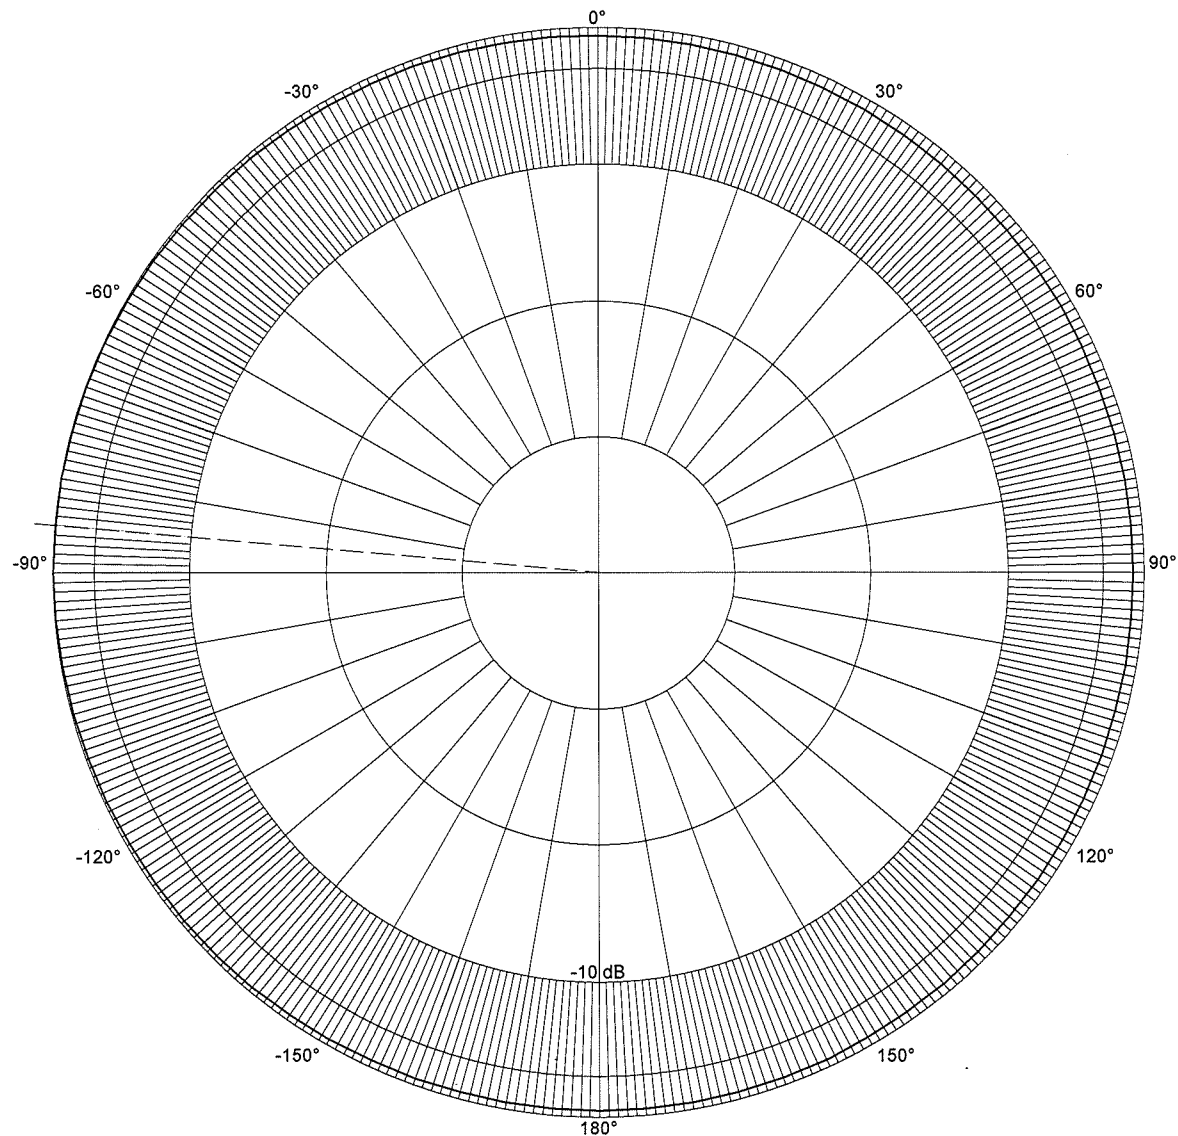




HYDROPHONE DIRECTIVITY

Under Test: TC4013-4
S/N: 0515084
Reference: TC4033
Date: 2015-04-01
Session, Run: 22116, 9
Max RR: -210.3 dB re 1 μ Pa/V at 1m
W: 342.9°
Comment: Vertical.

Amplitude: 10.0 Vrms
Pulse Width: 150.0 μ s
Angle: -180.0° to 180.0°
Frequency: 100.00 kHz

Temperature: 21.72°C
Depth: 1.2 m
Distance: 0.50 m
Tested by: PRA

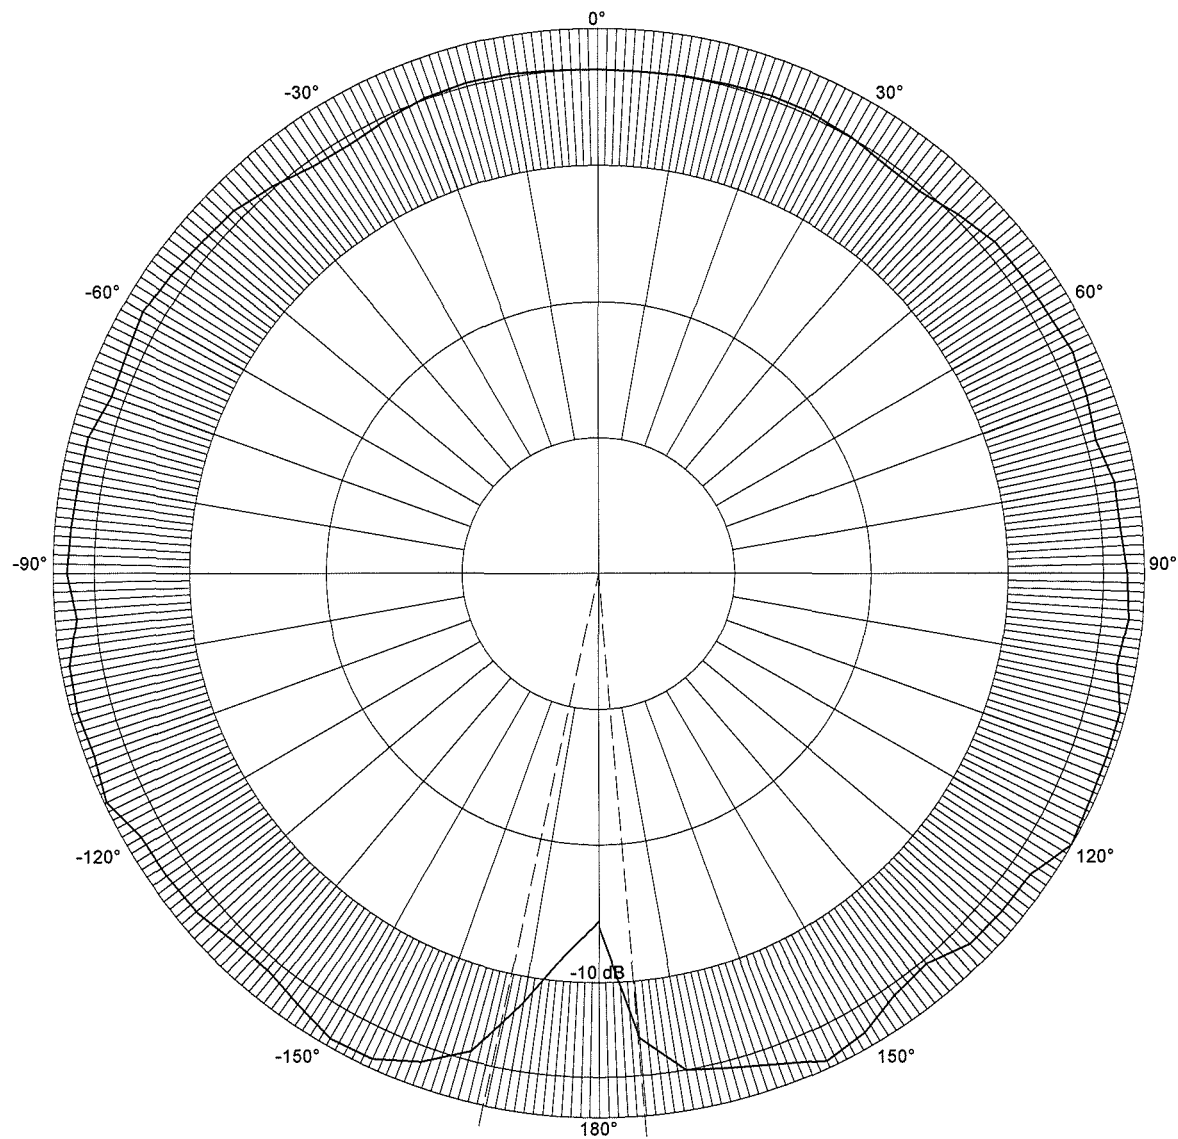




HYDROPHONE SENSITIVITY

Under Test: TC4013-4
S/N: 0515084
Reference:
Date: 2015-04-01
Session, Run: 22116, 2
Comment: PHO @ 250 Hz: -212.8 dB.

Amplitude: 25.0 Vrms
Pulse Width: 1400.0 μ s
Rep Rate: 66.7 ms
Averages: 8

Temperature: °C
Depth: 0.0 m
Distance: 0.00 m
Tested by: PRA

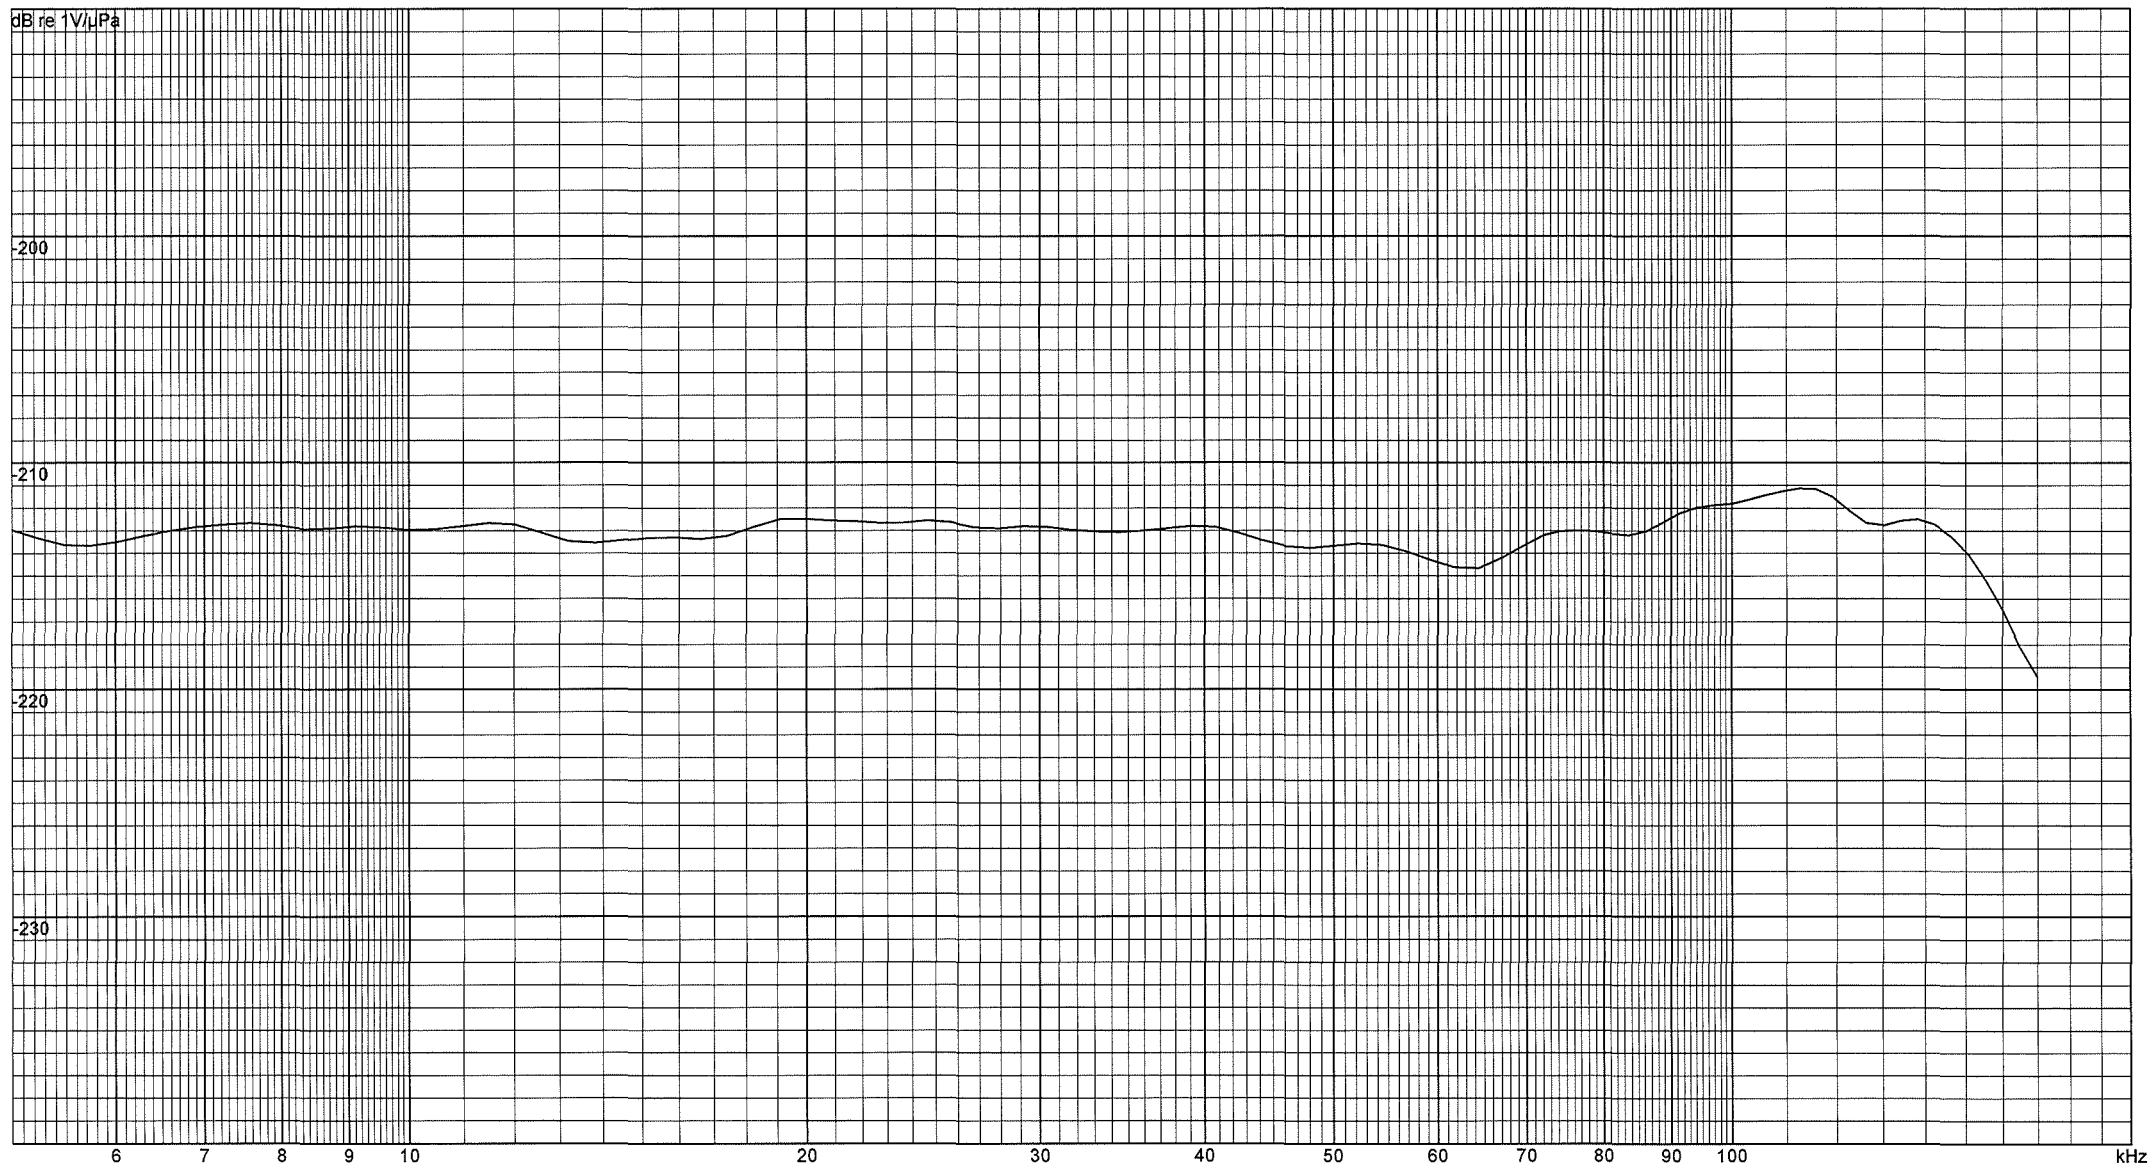




PROJECTOR SENSITIVITY

Under Test: TC4013-4
S/N: 0515084
Reference:
Date: 2015-04-01
Session, Run: 22116, 5
100.00 kHz: 130.71 dB re 1 μ Pa/V at 1m
Comment:

Amplitude: 20.0 Vrms
Pulse Width: 1400.0 μ s
Rep Rate: 100.0 ms
Averages: 8

Temperature: °C
Depth: 0.0 m
Distance: 0.00 m
Tested by: PRA

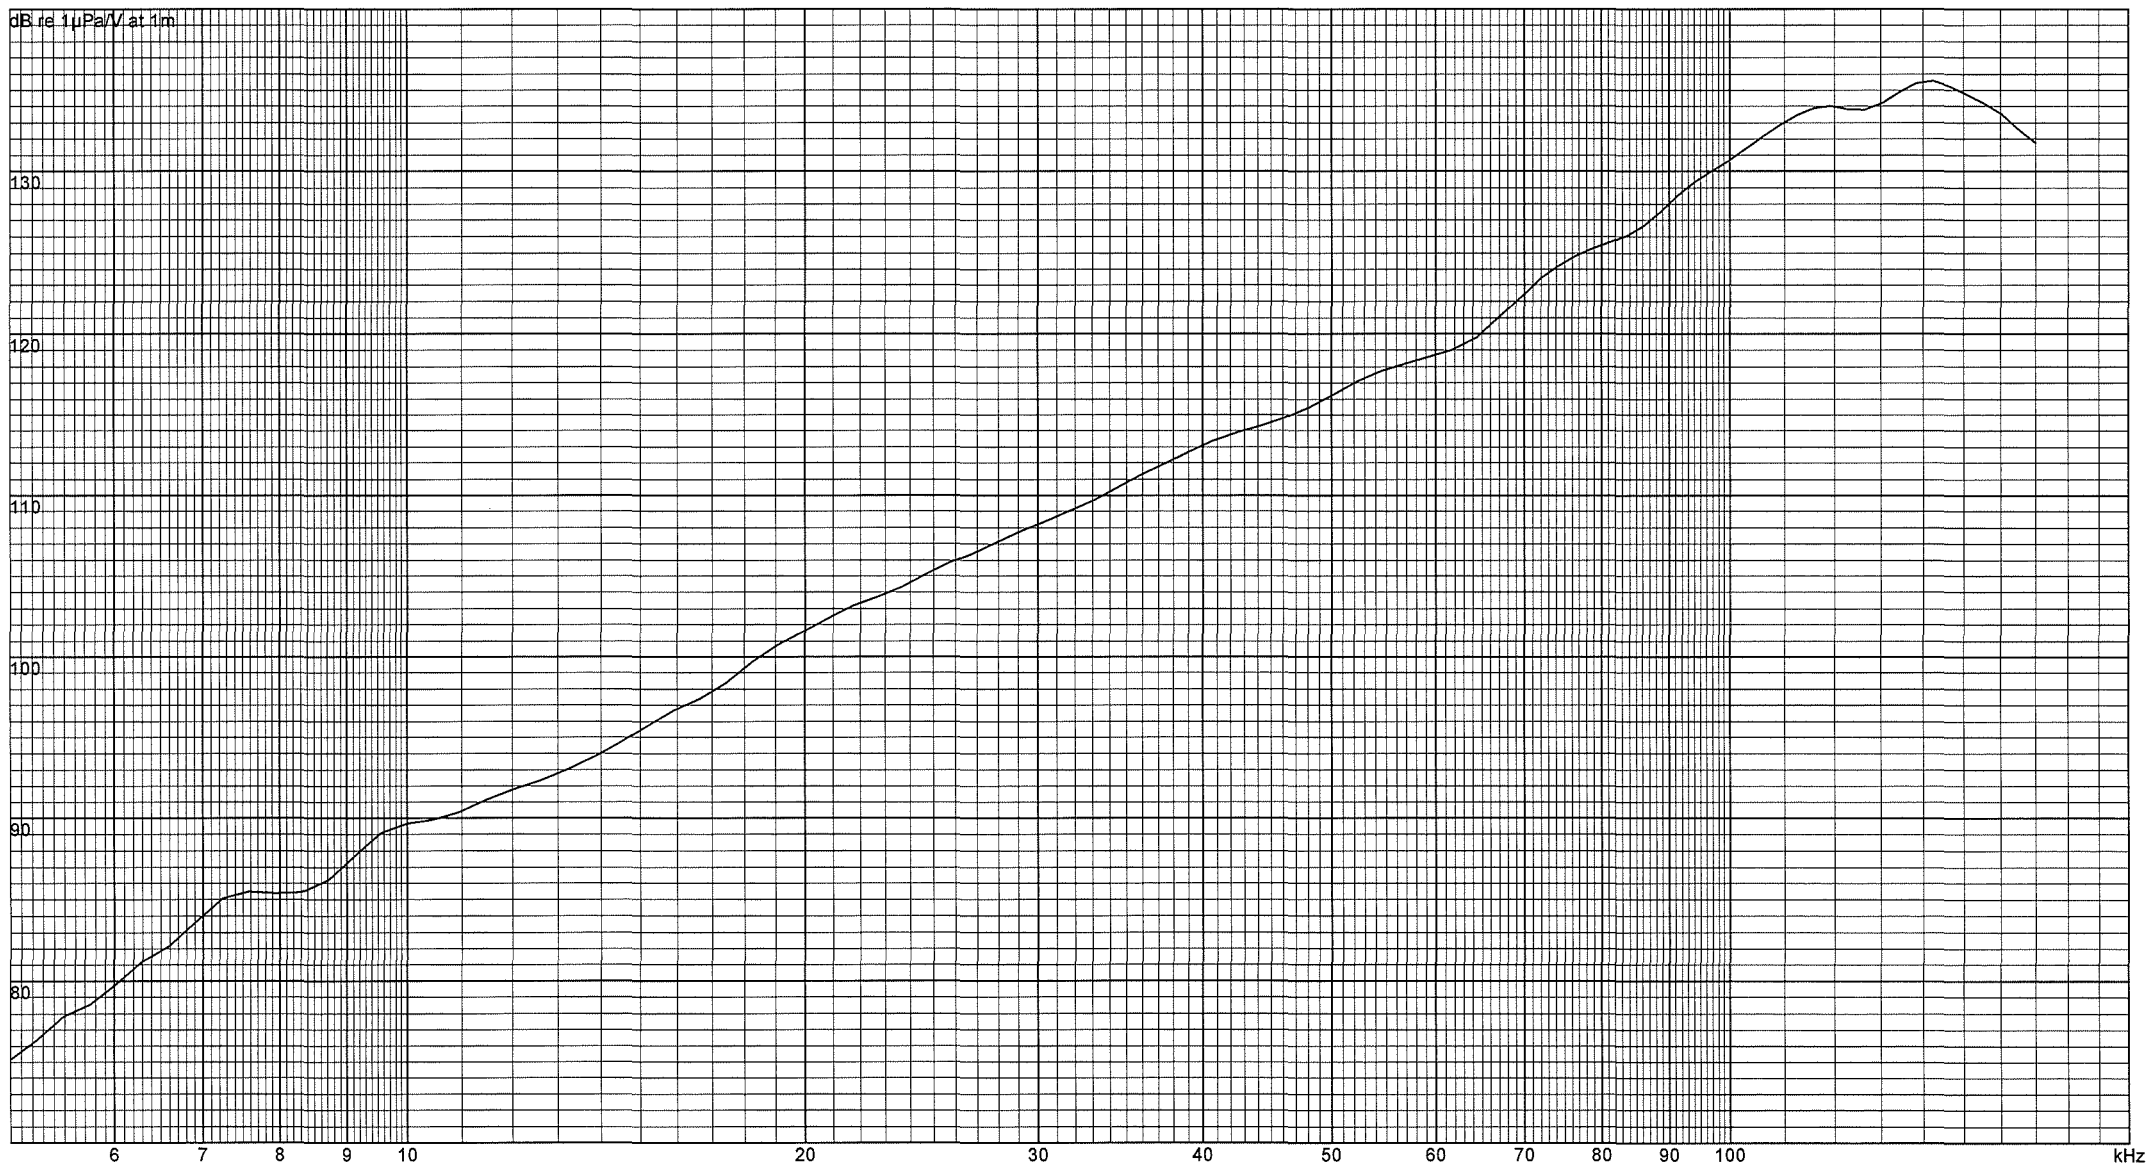



Under Test: TC4013-4
S/N: 0515084
Date: 2015-04-01
Session, Run: 22116, 6
Comment:

IMPEDANCE SUMARY

Amplitude: 10.0 Vrms
Pulse Width: 3000.0 μ s
Rep Rate: 33.3 ms
Averages: 4

Temperature: 21.72°C
Depth: 1.2 m
Cal Resistor: 0.0 ohms
Tested by: PRA

